


# GUIDANCE FOR CEMENTING PRIMARY TOTAL KNEE REPLACEMENTS

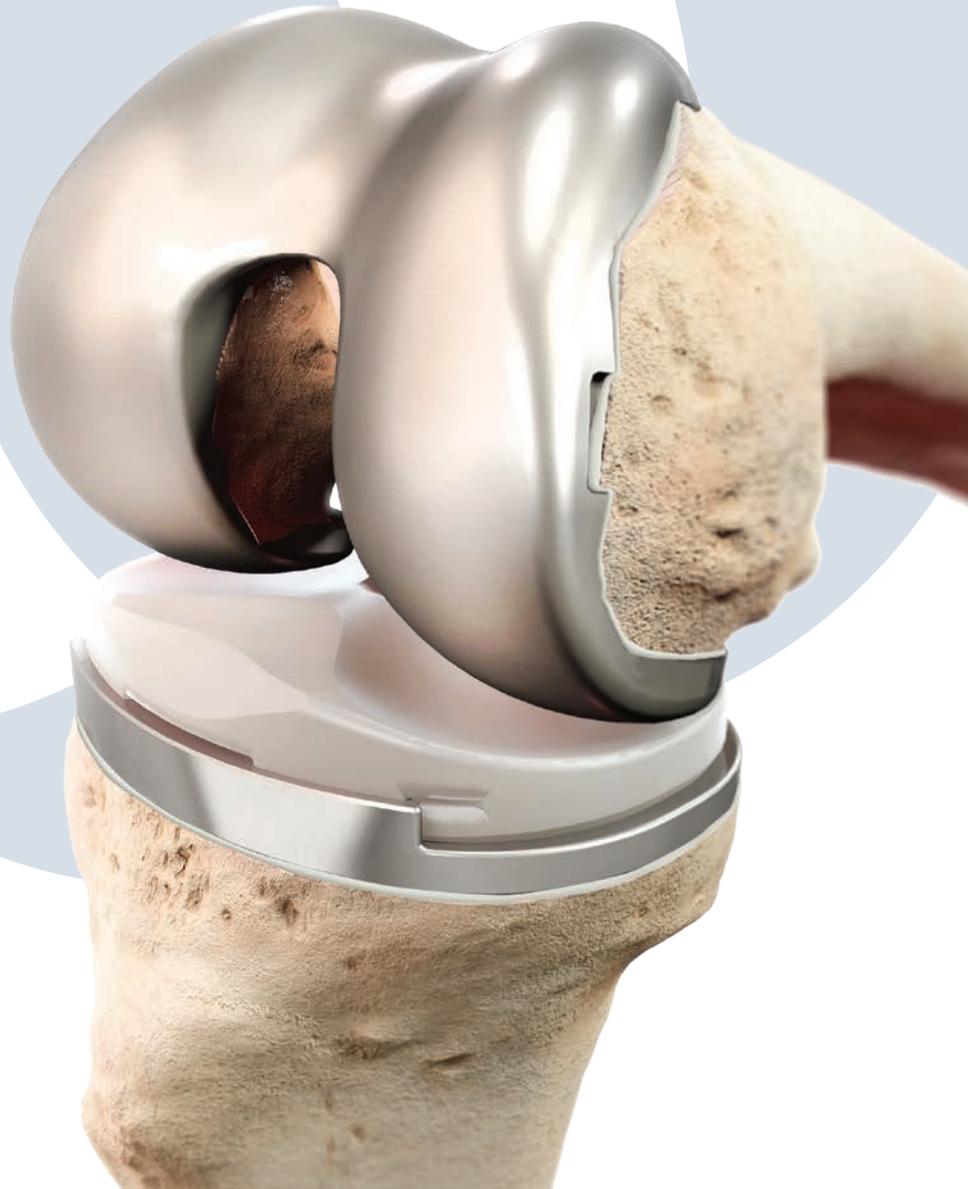

# CEMENTING PRIMARY TOTAL KNEE REPLACEMENTS

---

## 1.0 INTRODUCTION

The survivorship of Total Knee Replacement (TKR) is dependent on, among other factors, the cementing technique used.<sup>1</sup> Early attempts to use acrylic cement in orthopaedic surgery may have failed due to a misunderstanding around how the cement functions.<sup>2</sup> Cement achieves a mechanical bond to the bone by penetrating into the pores of the cancellous bone where it hardens, forming a micro-interlock; modern cementing techniques aim to improve this micro-interlock.

There are different cement considerations for TKR and Total Hip Replacement (THR). However, like in THR surgery, knee implants are known to fail at the cement-bone interface or at the cement-implant interface. Failure at the cement-bone interface may appear as radiolucent lines and is usually attributed to poor penetration of the cement into the bone.<sup>3</sup> Failure for the cement-implant interface may be due to the poor interfacial strength of the cement to the implant.<sup>4</sup>

## 2.0 DEFINITIONS

- **Dough time** – the change in physical condition of the cement identified by an increase in cement viscosity (becoming less runny), a change to a dull appearance, and reduced tackiness against surgical gloves.
- **Working time** – sometimes referred to as “dough state” – the optimum period of time for implanting the cement, this encompasses the time from when the dough state begins through final pressurization. This can be established for a given ambient temperature according to its specific instructions for use (package insert).
- **Ambient temperature** – the temperature of the surrounding environment in the operating room.
- **Working time/temperature chart** – a chart contained in the instructions for use (package insert) that defines the available working time for a given ambient temperature.

- **Final pressurization** – the final application of pressure to securely seat the implant within the bone cement by means of bringing the knee, with the implant, into extension and holding it there until the cement cures.
- **Cement setting or curing time** – is the time when the cement hardens.

## 3.0 GENERAL CEMENTATION PRINCIPLES

### 3.1 Cement Viscosity

Following mixing, all bone cements reach a higher viscosity state (dough state) and Medium Viscosity (MV) cements reach that higher dough state somewhat later than High Viscosity (HV) cements. In doing so MV cement is sometimes classified as having dual phases i.e. low viscosity (prior to reaching its dough state) and MV (once the dough state has been reached).

HV cements reach dough state quickly after mixing, and therefore do not have a low viscosity state. Care should be taken to use the HV cement immediately from the start of its dough time, and within its working time. The optimum time for cement application in TKR surgery is as soon as the cement has reached this dough state (i.e. as soon as the surface of the cement becomes less sticky even though the main body of the cement remains sticky).

- Application of the cement to the roughened implant surface early in the dough state has been demonstrated to increase the fixation strength of the cement to the implant.<sup>4</sup> It is therefore a general principle that cement should be applied to all cemented TKR components early on in the procedure; in some cases this will be several minutes before actual implantation into the bone.<sup>4</sup>
- Using the cement too early prior to the dough state may lead to poor pressurization and reduced penetration.<sup>5</sup>
- Using the cement too late in the dough state may reduce the flow of the cement into the bone and reduce penetration; it may also reduce the interfacial strength of the cement with the implant.<sup>4</sup>

## CEMENTING PRIMARY TOTAL KNEE REPLACEMENTS



Example of cement reaching dough state

The behavior of cement is strongly temperature sensitive; increasing the cement's temperature will speed up the curing of the cement, leading to an earlier dough-time and significantly reduced available working time.

**NOTE: The user should refer to the specific instructions for use (package insert) for the timing and usage chart before preparing the cement.**

**NOTE: Pre-warming powder or liquid beyond the temperature range stated in the instructions for use (package insert) is not recommended as it increases the risk of the cement being used too late in its working time phase.**

**NOTE: Heating MV cements will reduce the dough time (time to achieve dough state), however, heating HV cements will also reduce the available working time.**

**NOTE: When using a High Viscosity bone cement, it is advised to firmly apply the cement onto the implant early in its working phase by using a suitable cement gun, syringe, or spatula to encourage prime adhesion to the implant.**

### 3.2 Preparing Cement

When mixing cement, all of the powder must be mixed with all of the liquid to ensure that the cement behaves as intended. The cement is ready to use at the beginning of the dough state; when its appearance becomes dull and it is not excessively runny (or has excessive flow from the nozzle when using a syringe).

Example of mixing cement under vacuum



- Voids in the cement can reduce the strength of the cured cement<sup>6</sup>; mixing in a vacuum system reduces the inclusion of air voids<sup>7</sup> with the added benefit of reducing exposure to monomer fumes for OR staff.

**NOTE: Mixing under vacuum can impact the setting time and reference should be made to the instructions for use (package insert) for the relevant product.**

### 3.3 Working with Cement

The mixed cement in its working phase is incompatible with water and so aqueous liquids, such as saline or blood, will reduce its bonding strength.<sup>8,9</sup>

- Blood laminations in the cement can reduce the mechanical strength of the cement.<sup>9</sup> It is recommended to use clean gloves when cementing and all implant surfaces should be clean and dry. The use of a haemostatic agent (e.g. a solution containing H<sub>2</sub>O<sub>2</sub>) has been suggested to reduce the amount of blood and debris trapped within the trabecular bone-cement interface and may assist in reducing the risk of blood laminations.<sup>10</sup>

## 4.0 CEMENTATION IN TKR SURGERY

Because of the high range of complex movement in the knee following TKR, the cement mantle is subject to a wide range of forces. Although cement is strong in compression, the shear strength of the cement-bone interface is dependent on the depth of penetration. The strength of this interface is therefore dependent on cementation technique and an ideal depth of cement penetration into the bone of 3-4 mm has been proposed.<sup>11,12</sup>

### 4.1 Preparation of the Bone Surfaces

Washing all the bone surfaces (e.g. with pulsatile lavage) to remove loose bone, blood, fat, and marrow also exposes the porous bone and helps to achieve penetration of bone cement<sup>13</sup> resulting in a stronger interlock at the bone-cement interface.<sup>14</sup> The bone and implant should be dried prior to applying the cement; this may be achieved by drying in various ways including using an absorbent pad, such as a dry sponge, suction, or a carbon dioxide jet.

## CEMENTING PRIMARY TOTAL KNEE REPLACEMENTS

- In areas of dense or sclerotic bone, drilling keying holes in the bone may assist in creating a greater degree of cement interdigitation.<sup>15</sup>



Example of drilling keying holes in the tibial bone

### 4.2 Cement Application

A number of application techniques have been used to improve cement penetration:

- Cement can be syringed under pressure, by seating the nozzle directly onto the cut bone surface and syringing the cement into the cancellous bone structure. A purposefully designed tibial syringe applicator may be attached to the nozzle to facilitate this. Syringing cement in this way may provide an improved peripheral seal to retard later ingress of osteolytic micro-particulate debris into the bone, particularly at the periphery of the tibia.<sup>16</sup>

Examples of knee nozzles



- For MV cement, when in its low viscosity state, some surgical techniques use suction to improve penetration (especially in the tibial keel hole), additional cement is then applied to the bone surface.<sup>15</sup>
- In its dough state, MV cement and HV cement may be pressurized digitally, or by hand, into the bone surface.<sup>17</sup>
- Once the implant has been seated, an impactor can be used to help pressurize the cement.

- A thin layer of cement may not be sufficient to achieve good penetration into the bone. Sufficient cement must be applied and two mixes of standard (40g) packs of cement are often used in cementing



Example of one standard 40g pack of cement

the femoral and tibial components of a TKR to provide an adequate layer to facilitate cement pressurization. One 20g pack of cement is sufficient when cementing the patella alone.


## CEMENTING PRIMARY TOTAL KNEE REPLACEMENTS

### 4.3 Implantation

**NOTE: The surgeon should follow the implant system's surgical technique guidelines for applying cement to the knee components.**

During implantation, cement must flow from around the periphery of the implant to generate an adequate seal between the implant and bone; this is important in preventing later ingress of osteolytic particles and debris. However, it is extremely important to remove excess cement from around the implant. By using the cement according to the instructions for use (working time for a given ambient temperature) and by watching for the changes indicating initiation of the dough state, the cement will be in the appropriate portion of the dough state for both implantation and cleanup. Cement in the dough state can be pulled cleanly away from the bone. Cements used prior to the dough state can be more difficult to clean off the bone and soft tissues.

- Care must be taken not to pull cement from under the edge of the implant in order to ensure the edges remain sealed.

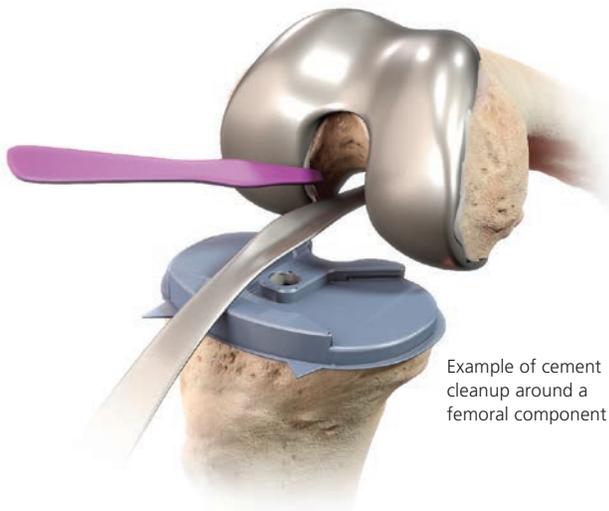

Example of cement cleanup around a femoral component

- Excess cement or cement debris not removed may scratch the implant and may lead to polyethylene wear debris.<sup>18</sup>



Example of cement cleanup around a femoral component

#### 4.3.1 Tibial Cementation

Generally the tibial component is cemented into place first and an impactor used to pressurize the cement. A number of different cementing techniques are known to be used. MV cement is sometimes applied soon after mixing and is poured onto the bone before its dough state is reached<sup>19</sup>, and the implant is seated onto the cement once it has reached the dough state. Alternatively, in the same way that the HV cement is frequently used, MV cement may be applied to the bone after it has reached its dough state. In this latter case a thick layer of cement should be applied to both the bone and implant surfaces. Cement should be applied to the cleaned and dried prepared tibial plateau, tibial stem, and to the undersurface of the tibial base.



Example of applying cement to both the tibial implant and bone

## CEMENTING PRIMARY TOTAL KNEE REPLACEMENTS

**NOTE: The surgeon should follow the implant system's surgical technique guidelines for applying cement to the tibial stem base.**

- If applying doughy cement to both the implant and bone, implantation should be completed early in its dough state to ensure good cement-cement adhesion and reduce the risk of dry laminations; which can weaken the cement.<sup>20</sup>

### 4.3.2 Femoral Cementation


A thick bed of cement may be placed onto the back of the implant or directly onto the exposed bone surface. An impactor is used to pressurize the cement. Good levels of penetration can be achieved by applying cement to the anterior and distal bone surfaces, and to the posterior flanges of the prosthesis prior to implantation.<sup>21</sup>



Example of applying cement onto the back of the femoral implant

- Retained posterior cement may prevent full flexion and generate debris so care must be taken to ensure posterior cleanout; despite the difficult access. Posterior extrusion may be reduced by applying posterior cement to the implant, rather than to the bone.

Example of using an impactor to implant and pressurize a femoral component

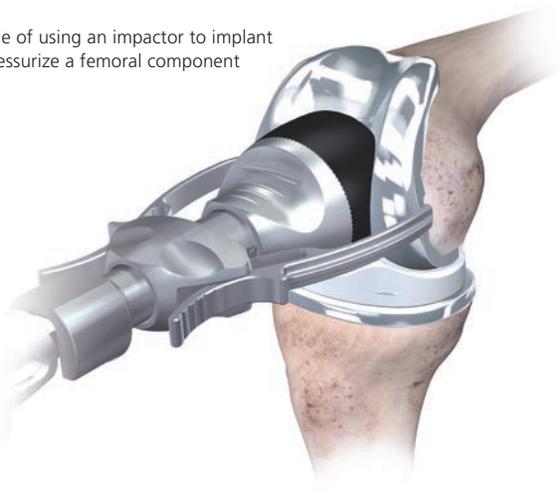

- For cementing a PS box, the general recommendation is to apply the cement to the implant, specifically the side walls of the PS box only, not to the top of the box; unless otherwise specified in the surgical technique.

**NOTE: Care should be taken to remove excess cement or cement debris which may scratch the implant which may lead to polyethylene wear debris.<sup>18</sup>**

### 4.3.3 Patella Cementation

If applying cement to the bone it should be pressed sufficiently into the bone surface and peg holes prior to introducing the patella implant. Alternatively, a thick bed of cement can be applied to the implant. A clamp is then used to fully pressurize the cement.



Example of using a patella clamp

## 5.0 FINAL PRESSURIZATION AND CLEANING

Once all components are implanted, extending the leg will further pressurize the cement while waiting for the cement to harden.

**NOTE: If the distribution of forces is unequal during final pressurization, the implants may move or cement may not penetrate into the cancellous bone equally in all zones<sup>3</sup> resulting in radiolucent lines and potentially early failure.**

**NOTE: This step will extrude excess cement: the knee must be examined and any extruded cement carefully removed.**

**NOTE: Care should be taken to apply bone cement to the patellar implant while the bone cement is in its working time, or dough phase.**

**NOTE: Keep the patella under compression, using the patella clamp, until the cement has fully hardened.**

## CEMENTING PRIMARY TOTAL KNEE REPLACEMENTS

---

### 6.0 SUMMARY AND CONCLUSION

The following is a summary of recommended TKR cementing practices:

- I.) Drill keyholes especially in areas of dense or sclerotic bone.
- II.) Thoroughly wash all bone surfaces before cementing.
- III.) Keep all surfaces clean and dry, including gloves, bone, and implant surfaces. Do not apply saline to the cement surface.
- IV.) Mix the cement under vacuum.
- V.) Use the cement within its working time.
- VI.) Do not preheat the powder or liquid, especially with HV type cements, as this may impact the available working time. Follow the appropriate instructions for use on cement preparation.
- VII.) Pressurize the cement by compression; use a thick layer of cement and impaction.
- VIII.) Ensure that cement around the periphery of the implant has been well pressurized into the bone.
- IX.) Remove all extruded cement around the implant, making sure the implant is sealed by cement around its edges.
- X.) Hold the cemented components under compression, until the cement is finally set; ensuring the components are properly balanced and do not move.

# CEMENTING PRIMARY TOTAL KNEE REPLACEMENTS

## 7.0 ORDERING INFORMATION

### SMARTSET® MV Bone Cement



Cat. No.	Description
3122-020	SMARTSET MV, 20g
3122-040	SMARTSET MV, 40g

### DePuy CMW 1



Cat. No.	Description
3312-040	DePuy CMW 1, 40g

### SMARTSET® HV Bone Cement



Cat. No.	Description
3092-020	SMARTSET HV, 20g
3092-040	SMARTSET HV, 40g

### DePuy CMW 1 Gentamicin Bone Cement



Cat. No.	Description
5450-31-500	DePuy CMW 1 Gentamicin, 40g

### SMARTSET® MV Endurance Bone Cement



Cat. No.	Description
3102-080	SMARTSET MV Endurance, 80g

### DePuy CMW 2



Cat. No.	Description
3322-020	DePuy CMW 2, 20g

### SMARTSET® GMV Bone Cement



Cat. No.	Description
5450-50-501	SMARTSET GMV Gentamicin, 40g

### DePuy CMW 2 Gentamicin Bone Cement



Cat. No.	Description
5450-32-500	DePuy CMW 2 Gentamicin, 20g

### SMARTSET® GHV Bone Cement



Cat. No.	Description
5450-35-500	SMARTSET GHV Gentamicin, 40g

### DePuy CMW 3



Cat. No.	Description
3332-040	DePuy CMW 3, 40g

## CEMENTING PRIMARY TOTAL KNEE REPLACEMENTS

---

### 8.0 REFERENCES

1. Philips, A. M., Tomlinson, E., Goddard, N. J. (1996). Current technologies in total knee replacement: Results of a national survey. *Annals of The Royal College of Surgeons of England*, 78, 515-520.
2. Charnley, J. (1972). *Acrylic cement in orthopaedics surgery*. Churchill Livingstone, 95.
3. Guha, A. R., Debnath, U. K., Graham, N. M. (2008). Radiolucent lines below the tibial component of a total knee replacement (TKR) - a comparison between single- and two-stage cementation techniques. *International Orthopedics*, 32 (4): 453-457.
4. Shepard, M. F., Kabo, J. M., Liebermann, J. R. (2000). Influence of cement technique on the interface strength of femoral components. *Clinical Orthopaedics and Related Research*, Number 381, 26-35.
5. Breusch, S., Heisel, C., Müller, J., Borchers, T., and Mau, H. (2002). Influence of cement viscosity on cement interdigitation and venous fat content under in vivo conditions: A bilateral study of 13 sheep. *Acta Orthopaedica Scandinavica*, 73 (4): 409-415.
6. Lidgren, L., Drar, H., Moller, J. (1984). Strength of polymethylmetacrylate increased by vacuum mixing. *Acta Orthopaedica Scandinavica*, 55 (5): 536-541.
7. Alkire, M., Dabezies, E., Hastings, P. (1987). High vacuum as a method of reducing porosity of polymethylmethacrylate. *Orthopedics*, 10: 1533-1539.
8. Rudol, G., Wilcox, R., Jin, Z., Tsiridis, E. (2011). The effect of surface finish and interstitial fluid on the cement in cement interface in revision surgery of the hip. *The Journal of Bone and Joint Surgery. British Volume*. 93 (2): 188-193.
9. Jansson, V., Zimmer, M., Kühne, J. H., Ishida, A. (1993). Blood lamination in bone cement--effect of cementing technique. *Der Unfallchirurg*, 96 (7): 390-394.
10. Hankin, F. M., Campbell, S. E., Goldstein, S. A., Matthews, L. S. (1984). Hydrogen peroxide as a topical hemostatic agent. *Clinical Orthopaedics and Related Research*, (186): 244-248.
11. Walker, P., Soudry, M., Ewald, F., McVickar, H. (1984). Control of cement penetration in total knee arthroplasty. *Clinical Orthopaedics Related Research*, 185: 155-164.
12. Lutz, M. J., Pincus, P. F., Whitehouse, S. L., Halliday, B. R. (2009). The effect of cement gun and cement syringe use on the tibial cement mantle in total knee arthroplasty. *The Journal of Arthroplasty*, 24 (3): 461-467.
13. Majokowski, R. S., Miles, A. W., Bannister, O. C., Perkins, J., Taylor, G. J. S. (1993). Bone surface preparation in cemented joint replacement. *The Journal of Bone and Joint Surgery*, 75 (3): 459-463.
14. Ravenscroft, M. J., Charalambous, C. P., Mills, S. P., Woodruff, M. J., Stanley, J. K. (2010). Bone cement interface strength in distal radii using two medullary canal preparation techniques: Carbon dioxide jet cleaning versus syringed saline. *Hand Surgery*, 15 (2): 95-98.
15. Rauh, M. A., Clark, L. D., Shah, H., Krackow, K. A., Mihalko, W. M. (2008). The effect of drill hole size on the fixation strength of a cemented prosthetic patellar button. *Orthopedics*, 31 (6): 541.
16. Dennis, D. A. (2008). Surgeon offers advice for optimal cement fixation in primary total knee arthroplasty. *Orthopedics Today*. Retrieved from <http://www.healio.com/orthopedics/kneenews/print/orthopedics-today>
17. Norton, M. R., Eyres, K. S. (2000). Irrigation and suction technique to ensure reliable cement penetration for total knee arthroplasty. *The Journal of Arthroplasty*, 15 (4): 468-474.
18. Currier, J. H., Porter, E. C., Mayor, M. B., Collier, J. P., Van Critters, D. W. (2011). Damage and wear: An important distinction in rotating platform knee bearings. *Journal of ASTM International*, 8 (2).
19. Cawley, D. T., Kelly, N., McGarry, J. P., Shannon, F. J. (2013). Instructional review: Knee cementing techniques for the tibial component in primary total knee replacement. *The Bone and Joint Journal*, 95-B: 295-300.
20. Park, S. H., Silva, M., Park, J. S., Ebrahimzadeh, E., Schmalzried, T. P. (2001). Cement interface strength: Influence of time to apposition. *Journal of Biomedical Materials Research*, 58 (6): 741-746.
21. Vaninbrouckx, M., Labey, L., Innocenti, B., Bellemans, J. (2009). Cementing the femoral component in total knee arthroplasty: Which technique is the best? *The Knee*, 16 (4): 265-8.

**Limited Warranty and Disclaimer:** *DePuy Synthes Companies* products are sold with a limited warranty to the original purchaser against defects in workmanship and materials. Any other express or implied warranties, including warranties of merchantability or fitness, are hereby disclaimed.

**WARNING:** In the USA, this product has labeling limitations. See package insert for complete information.

**CAUTION:** USA Law restricts these devices to sale by or on the order of a physician.

Not all products are currently available in all markets.



**DePuy Orthopaedics, Inc.**  
700 Orthopaedic Drive  
Warsaw, IN 46582  
USA  
T. +1 (800) 366-8143

[www.depuyorthos.com](http://www.depuyorthos.com)

**DePuy (Ireland)**  
Loughbeg Ringaskiddy  
Co. Cork  
Ireland  
Tel: +35 (321) 491-4278  
Fax: +35 (321) 491-4199

**DePuy International Ltd.**  
St. Anthony's Road  
Leeds LS11 8DT  
England  
Tel: +44 (113) 270-0461  
Fax: +44 (113) 272-4101

